

Moisture meter

Operating Manual

humimeter FL2

Moisture meter with insertion probe


for measuring the moisture content of hay and straw



78,0°F | 6,16% | 456kg/m³ | -27,3td | 0,64aw | 51,9%r.H. | 14,8%abs | 100,4g/m² | 09m/s | 4,90Ugl | 1

Your humimeter FL2 at a glance

The main unit

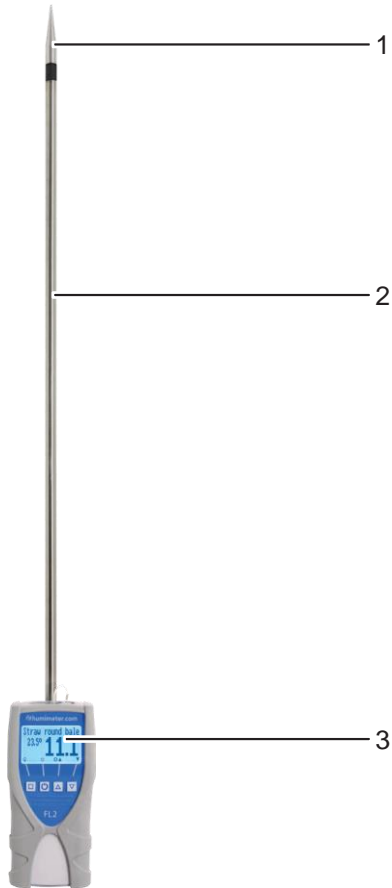


No	Name
1	Measuring head
2	Insertion probe
3	Electronics in plastic housing

The main unit in detail




No	Name
1	USB port (optional)
2	Display
3	Keypad
4	Rubber protection cover

Rear of the main unit

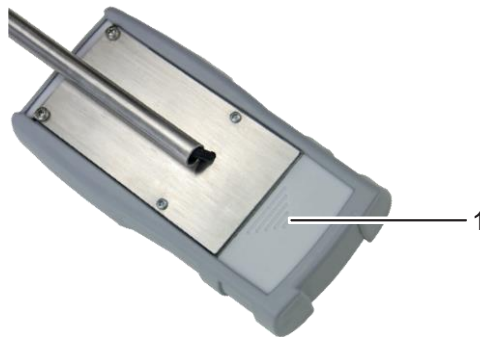


No	Name
1	Battery compartment

The measuring head

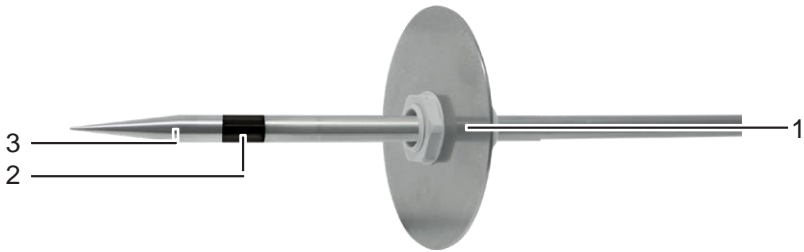





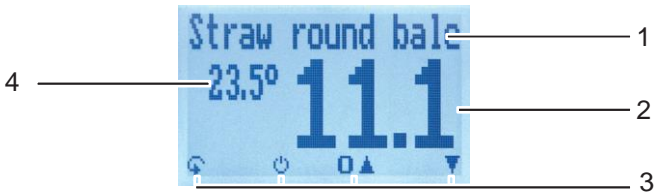













No	Name
1	Compression plate
2	Isolator
3	Measuring tip

The display



No	Name
1	Calibration curve
2	Moisture content % (" 6.2 How moisture is defined ")
3	Display symbols
4	Temperature display


The display symbols

Symbol	Name	Symbol	Name
	Enter		No
	Up		Change input level
	Down		OK
	Back		Change menu
	Enter numbers		Enter data
	Enter letters		View measurements
	Continue / go right		Delete measurements
	Left		On/off button, display light
	Yes		Save measured value

The menus


The device has three different menus: product selection, Data Log and main menu:

Product selection menu



No	Name
1	Change menu
2	Display illumination / device on/off
3	For changing the calibration curve

Data Log menu



No	Name
1	Change menu
2	Display illumination / device on/off
3	Save measured value
4	Show the last recorded values

Main menu

The main menu comprises the following menu items:

- **Edit Logs:**
Manual Logs, Clear Logs
- **Print Logs:**
Last Log, All Logs, Clear Logs
- **Send Logs:**
Manual Logs, Clear Logs
- **Options:**
Bluetooth, Date/Time, Log Time, Language, Unlock, °C/°F, Userlevel, BL On Time, Auto Off Time, Materialcalib., Online Send, Password, Reset
- **Status**

Table of contents

Your humimeter FL2 at a glance	2
The main unit	2
The main unit in detail	3
Rear of the main unit.....	3
The measuring head	4
The display	4
The menus.....	5
1. Introduction.....	11
1.1 Information about this operating manual	11
1.2 Limitation of liability	11
1.3 Symbols used in this manual	12
1.4 Customer service	12
2. For your safety.....	13
2.1 Proper use.....	13
2.2 Improper use.....	13
2.3 User qualifications	13
2.4 General safety information	14
2.5 Warranty.....	14
3. On receipt of your device.....	15
3.1 Taking the device out of its packaging	15
3.2 Making sure that all of the components have been included.....	15
3.3 Inserting batteries	16
4. Using the device - Basics	16
4.1 Switching the device on.....	16
4.2 Selecting the calibration curve.....	17
4.3 Taking a measurement	17
4.4 Switching the device off	17

5.	The measuring process	18
5.1	Preparing a measurement	18
5.1.1	Measuring loose hay/straw	18
5.2	Taking a measurement	19
5.2.1	Measuring hay and straw bales	19
5.2.2	Measuring loose hay/straw	19
5.3	Simplified user	21
5.3.1	Activating/deactivating the simplified user	21
5.3.2	Using the simplified user	21
5.4	Hold function - Freezing the displayed values	21
5.4.1	Activating the hold function in the options menu	21
5.4.2	Using the hold function	22
5.5	Saving individual readings	22
5.5.1	Activating the manual saving function in the options menu	22
5.5.2	Using the manual saving option	23
5.6	Saving several readings (a measurement series) at the same time	24
5.7	Viewing individual readings	26
5.8	Viewing individual readings from a series of measurements	26
5.9	Deleting all measured values (data log)	27
5.10	Deleting individual measurement series	27
5.11	Deleting single values from a series of measurements	28
6.	Calibration curves	29
6.1	Digit calibration curve	29
6.2	How moisture is defined	30
6.3	Selecting the calibration curve	30
6.4	Notes for comparative measurement with oven-drying method	32
7.	Using the LogMemorizer program	33
7.1	Installing / opening the program	33
7.2	Exporting measured values to a computer	34

8.	Checking on the device's status	36
9.	Configuring the device	37
9.1	Turning on Bluetooth	37
9.2	Adjust the date/time	37
9.3	Selecting a language	38
9.4	Activating options.....	38
9.5	Deactivating options	39
9.6	Selecting °C/°F	39
9.7	Changing the Userlevel	40
9.7.1	Changing from advanced to simplified user	40
9.7.2	Changing from simplified to advanced user	40
9.8	Reducing the device's power consumption	41
9.8.1	Configuring the display illumination time.....	41
9.8.2	Configuring automatic switch-off	41
9.9	Configuring the material calibration function.....	42
9.10	Changing the password	42
9.11	Resetting the device to its factory settings.....	43
10.	Cleaning and maintenance	43
10.1	Changing batteries	43
10.2	Care instructions.....	44
10.3	Cleaning the device	44
11.	Faults	45
12.	Storage and disposal	47
12.1	Storing the device.....	47
12.2	Disposing of the device	47
13.	Device information	48
13.1	CE declaration of conformity.....	48
13.2	Technical data	52

14.	Notes	53
------------	--------------------	-----------

1. Introduction

1.1 Information about this operating manual

This operating manual is designed to enable you to use the humimeter FL2 safely and effectively. It is part of the device, has to be stored nearby and must be easily accessible to users at all times.

All users are required to carefully read and make sure that they have understood this operating manual before using the humimeter FL2. All of the safety and operating instructions detailed in this manual have to be observed to ensure the safety of the device.

1.2 Limitation of liability

All of the information and instructions provided in this operating manual have been compiled on the basis of the current standards and regulations, the state of the art, and the extensive expertise and experience of Schaller Messtechnik GmbH.

Schaller Messtechnik GmbH does not accept any liability for damage associated with the following, which also voids the warranty:

- Non-observance of this operating manual
- Improper use
- Inadequately qualified users
- Unauthorised modifications
- Technical changes
- Use of unapproved spare parts

This fast measuring procedure can be affected by a range of different factors. For this reason, we recommend periodically checking the device's measurements with a standardised oven-drying method.

We as the manufacturer do not accept any liability for any incorrect measurements and associated consequential damage.

1.3 Symbols used in this manual

All the safety information provided in this manual is shown with a corresponding symbol.



CAUTION

It is essential to observe this warning. Non-compliance can lead to injury.



ATTENTION

It is essential to observe this warning. Non-compliance can lead to damage to property or equipment.



Information

This symbol indicates important information that enables users to use the device more efficiently and cost-effectively.

1.4 Customer service

For technical advice, please contact our customer service department at:

Schaller Messtechnik GmbH
Max-Schaller-Straße 99
A - 8181 St.Ruprecht an der Raab

Telefon: +43 (0)3178 28899
Fax: +43 (0)3178 28899 - 901

E-Mail: info@humimeter.com
Internet: www.humimeter.com



© Schaller Messtechnik GmbH 2024

2. For your safety

The device complies with the following European directives:

- Restriction of Hazardous Substances in Electrical and Electronic Equipment (RoHS)
- Electromagnetic compatibility (EMC)

The device corresponds to state-of-the-art technology. However, it is still associated with a number of residual hazards.

These hazards can be avoided through strict observance of our safety information.

2.1 Proper use

- Easy to use device for quickly measuring the moisture content of hay and straw
- The device must only be used for taking measurements on the products defined in the following sections of this manual (see "[6. Calibration curves](#)").

2.2 Improper use

- The device is not suitable for measuring mouldy or rain wet hay/straw.
- The device is not waterproof and must be protected from water and fine dust (IP40).

2.3 User qualifications

The device must only be operated by people who can be expected to reliably take the measurements. The device must not be operated by people whose reaction times may be slowed due to, e.g. the use of drugs, alcohol or medication.

All persons using this device must have read, understood and follow the instructions provided in the operating manual.

2.4 General safety information

The following safety information has to be observed at all times to avoid damage to objects and injury to people:

- Remove the batteries if the device isn't used for a prolonged period of time.
- Keep the measuring head away from your body throughout all activities.
- Keep the measuring head away from other people throughout all activities.
- In case of damages or loose parts on the device, remove the batteries and contact Schaller Messtechnik GmbH or your dealer.

All of the device's technical features have been inspected and tested before delivery. Every device has a serial number. Do not remove the tag with the serial number.

2.5 Warranty

The warranty does not apply to:

- Damage resulting from non-observance of the operating manual
- Damage resulting from third-party interventions
- Products that have been used improperly or modified without authorisation
- Products with missing or damaged warranty seals
- Damage resulting from force majeure, natural disasters, etc.
- Damage from improper cleaning
- Batteries older than six months
- Damage resulting from improper strain (pressure, bending) of the insertion probe or the measuring head
- Damage by dropping the measuring head

3. On receipt of your device

3.1 Taking the device out of its packaging

- Take the device out of its packaging.
- Next, make sure that it is not damaged and that no parts are missing.

3.2 Making sure that all of the components have been included

Make sure that all of the components have been included by checking the package contents against the following list:



- humimeter FL2
- 4 pieces of AA Alkaline batteries
- Rubber protection cover
- Compacting plate
- Wooden case
- Operating manual

Optional accessories:

- humimeter USB data interface module - USB flash drive with software and USB-cable or download using humimeter.com/software
- Battery operated portable thermal printer (only possible together with humimeter USB data interface module) - Described in a separate operating manual
- Bluetooth module (only possible together with humimeter USB data interface module) - Described in a separate operating manual
- Test block


3.3 Inserting batteries

1. Remove the rubber protection cover. To do so, hold the rubber protection cover at the upper side and pull it over. If your device is provided with an optional USB port, remove the protection cap of the USB socket before (figure 1 and 2).
2. Take hold of the device with one hand, press your thumb onto the engraved area of the battery compartment (1) and drag downwards (2) (figure 3).
3. Insert the batteries with negative and positive terminals matching those indicated on the battery compartment. Press down the batteries so that they lay flat on the bottom of the housing (figure 4).
 - » As soon as all batteries have been inserted, the device switches on automatically.
4. Push the battery cover onto the housing until it clicks into place. Then mount the rubber protection cover onto the housing, beginning at the end where the battery compartment is situated (figure 5).



4. Using the device - Basics

4.1 Switching the device on






- Press the  button for 3 seconds.
 - » The display will then show the status indicator (figure 6).
 - » After inserting the batteries, the device switches on automatically.




4.2 Selecting the calibration curve

To do so: The device has to be in the product selection menu (figure 7).

For an overview of the different calibration curves and the criteria for selecting them, please refer to "6. Calibration curves"es".

1. Press the  or  button to move from one product to the next Or
2. Press the  or  button for 3 seconds to open the calibration curve overview (figure 8).
3. Use the arrow keys to move from one calibration curve to the next
4. and keep any of them pressed to scroll through the types.
5. Confirm your selection by pressing .




» The calibration curve you selected will now be shown at the top of the display.

4.3 Taking a measurement

- For information on how to take a measurement, see section "5. The measuring process".

4.4 Switching the device off



To do so: The device has to be in the product selection, the Data Log or the additional function menu. It is not possible to switch off the device when it is in the main menu.


- Press the  button for 3 seconds.

5. The measuring process

5.1 Preparing a measurement

To do so: The device has to have nearly the same temperature than the product being measured. It is recommended to let your humimeter device adjust to the surrounding temperature before the measurement.


1. Switch on the device (see "4.1 Switching the device on").
2. Select the desired calibration curve (see "6. Calibration curves"es") by pressing the  or  (see "4.2 Selecting the calibration curve"rve") (figure 10).



5.1.1 Measuring loose hay/straw

Assembly of the compression plate

1. Loosen the fixing nut.
2. Guide the compression plate over the measuring head onto the insertion probe (figure 11).
 - » The fixing nut has to face towards the device.
3. Position the compression plate on the insertion probe and fasten the fixing nut by hand (figure 13).
 - » The recommended distance between isolator and compression plate amounts to approx. the length of the measuring tip (figure 14).
 - » The compression plate must not be moved by moderate contact pressure.



5.2 Taking a measurement

5.2.1 Measuring hay and straw bales

To do so: The device has to have nearly the same temperature than the product being measured.

- Insert the measuring head of the device straight into the hay or straw bale (figure 15).
 - » Do not bend or drop the measuring head!
 - » Both round bales and rectangle bales have to be measured on the face side of the bale!
- The device will now instantly display the moisture content on the display (figure 16).
 - » The displayed value flashes when the moisture content exceeds the measuring range of the selected calibration curve (figure 17). A flashing value signals lowered accuracy of the measurement. The measuring range is dependent on the calibration curve (see "6. Calibration curves"es").
 - » Once the reading has been taken, it can be saved on the device (see "5.5 Saving individual readings" or "5.6 Saving several readings (a measurement series) at the same time").



5.2.2 Measuring loose hay/straw

To do so: The device has to have nearly the same temperature than the product being measured. There has to be enough material to ensure adequate compaction.

1. Insert the measuring head of the device straight into the hay or straw (figure 18).
 - » Do not bend or drop the measuring head!
2. Use the insertion probe to collect material and compress it (figure 19 and 20).
 - » A contact pressure must be noticeable.
 - » The measuring tip must not penetrate into the ground.
3. While compacting, have an eye on the display.



- » Continue to compact as long as the display shows a constant measuring value (figure 21).
- » The displayed value flashes when the moisture content exceeds the measuring range of the selected calibration curve (figure 17). A flashing value signals lowered accuracy of the measurement. The measuring range is dependent on the calibration curve (see "6. Calibration curves"es").
- » Once the reading has been taken, it can be saved on the device (see "5.5 Saving individual readings" or "5.6 Saving several readings (a measurement series) at the same time").

20



21



CAUTION

Risk of injury

Risk of injury due to the measuring head

- ▶ Keep the measuring head away from your body throughout all activities.
- ▶ Keep the measuring head away from other people throughout all activities.



ATTENTION - HIGH MEASURING INTERVAL

The measuring head will heat up when taking a high amount of measurements on bales with high compressed density, in a rapid succession. This will decrease the accuracy of the measurement significantly.



Information - Measuring accuracy

This rapid and non-destructive measuring procedure allows you to take moisture readings at a number of different points. When saving the individual readings, the device will automatically calculate the readings' average (see "5.6 Saving several readings (a measurement series) at the same time").



Information - Incorrect readings

Always make sure to select the correct calibration curve for the material you are measuring. This prevents taking incorrect readings (see "11. Faults").

5.3 Simplified user

The device can be configured in such a way that the access of the user can be reduced to the product selection menu combined with the hold function.

5.3.1 Activating/deactivating the simplified user

- For information on how to activate/deactivate the simplified user, see section "9.7 Changing the Userlevel".

5.3.2 Using the simplified user

The simplified user offers the following limitations:

- The only useable menu is a slightly modified product selection menu (figure 22).
- » No access to the Data Log or main menu.
- Hold function replaces the function to switch between the different menus (see "5.4 Hold function - Freezing the displayed values").















5.4 Hold function - Freezing the displayed values



The device can be configured in such a way that the information being shown on the display will freeze at the touch of a button until a new button is pressed. This function can be very useful when e.g. taking readings in spaces where it is not possible to see the display (e.g. overhead).

5.4.1 Activating the hold function in the options menu

To do so: The device has to be switched on and be in the product selection menu.



1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Log Time** (figure 23). To do so, press  or  and confirm by pressing .
4. Select **Hold** (figure 24). To do so, press  or  and confirm by pressing .
- » The setting has been saved.



5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

5.4.2 Using the hold function

To do so: The device has to be switched on and be in the Data Log menu (see "The menus" page 5).

- Press .
- » The current reading will be frozen. All of the four symbols will now be displayed as  (figure 25).
- To reactivate the frozen display, simply press any button.

















5.5 Saving individual readings

The device can be configured in such a way that the device will save a reading every time a button is pressed. This option (manual saving function) is the device's default setting.

5.5.1 Activating the manual saving function in the options menu











To do so: The device has to be switched on and be in the product selection menu.


1. Press  twice or hold for 2 seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Log Time** (figure 26). To do so, press  or  and confirm by pressing .
4. Select **Manual** (figure 27). To do so, press  or  and confirm by pressing .
- » The setting has been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.



5.5.2 Using the manual saving option



To do so: The device has to be in the Data Log menu (see "The menus" page 5). The device is set to Data Log time - Manual.

1. Press .
 - » The display will now appear as shown in figure 29 and the disc symbol will be preceded by the digit one.
2. Press  to enter a name for the saved reading and to finish the measuring process.
 - » The display will now appear as shown in figure 30.
3. The data you have inputted can be overwritten at any time.
4. **Inputting letters:**
Press and hold  to quickly scroll to the required letter and either press it for 3 seconds or press  to confirm the selected letter (figure 31).
5. **Inputting numbers:**
Press and hold  to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number.
6. **Moving forward/back:**
Press  to switch to another input level. Press  or  to move forward or back.
7. Confirm your entry by pressing .
 - » The data you entered has been saved.




5.6 Saving several readings (a measurement series) at the same time


To do so: The device has to be in the Data Log menu (see "Data Log menu" page 6).


1. Take several measurements at different points of the same haystack (see "5. The measuring process").
 2. After each measurement, press  to save the reading.
- » The display will appear as shown in figure 32. The marked number shows the number of readings that have already been saved.
3. Press  to enter a name for the saved measurement series and to finish the measuring process.







- » The display will now appear as shown in figure 33.
4. The data you have inputted can be overwritten at any time.




5. **Inputting letters:**
Press and hold **A..Z** to quickly scroll to the required letter and either press it for 3 seconds or press  to confirm the selected letter (figure 34).



6. **Inputting numbers:**
Press and hold **0..9** to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number.

7. **Moving forward/back:**
Press  to switch to another input level. Press  or  to move forward or back.

8. Confirm your entry by pressing .
 - » The data you entered has been saved.
 - » The device automatically determines the average moisture content of the saved measuring values.





» The display will show the following information:




No	Name
1	Name of the measurement series (editable)
2	Temperature (average)
3	Date & start time of the measurement series
4	Date & end time of the measurement series
5	Number of saved readings
6	Calibration curve
7	Device name
8	Moisture content (average)

5.7 Viewing individual readings









To do so: You must have saved a reading (e.g. **1 Log**). The display will now appear as shown in figure 35.


1. Press .
2. Select the required reading. To do so, press  or .
 - » The display will now appear as shown in figure 36.
 - » Press  to leave this screen.



5.8 Viewing individual readings from a series of measurements











To do so: You must have saved a series of measurements (e.g. **2 logs**). The display will now appear as shown in figure 37.



1. Press .
2. Navigate to the required measurement series. To do so, press  or .
 - » The display will now appear as shown in figure 38.
3. Press  to switch to another input level.
 - » The display will now appear as shown in figure 39.
4. Press  again.
 - » The display will now appear as shown in figure 40.
5. Navigate to the required reading (**No.: 1, No.: 2, No.: 3**). To do so, press  or .
6. Press  to leave this screen.



5.9 Deleting all measured values (data log)






To do so: You must have taken and saved one or several readings.


1. Press  twice or hold for 2 seconds.
2. Select **Edit Logs** (figure 41). To do so, press  or  and confirm by pressing .
3. Select **Clear Logs** (figure 42). To do so, press  or  and confirm by pressing .
 - » The display will show the message **clear?** (figure 43).
4. Confirm by pressing .
 - » The data log has been deleted.
5. Press  to leave the **Edit Logs** menu.
6. Press  to leave the main menu.



5.10 Deleting individual measurement series

To do so: You must have saved a measured value (e.g. **1 log**) or a series of measurements (e.g. **3 logs**). The display will now appear as shown in figure 44.


1. Press .
 - » The display will now appear as shown in figure 45.
2. Select the required reading. To do so, press  or .
3. Press  to switch to another input level.
 - » The display will now appear as shown in figure 46.
4. Press .



- » The display will then show the message **clear?** (figure 47).

5. Confirm by pressing .

- » The value has been deleted.





5.11 Deleting single values from a series of measurements

To do so: You must have saved a series of measurements comprising of at least 2 logs. The display will now appear as shown in figure 48.

1. Press .

- » The display will now appear as shown in figure 49.



2. Select the required reading. To do so, press  or .


3. Press  to switch to another input level.

- » The display will now appear as shown in figure 50.

4. Press .

- » The display will now appear as shown in figure 51.

5. Select the required measured value. To do so, press  or .

6. Press  to switch to another input level.




- » The display will now appear as shown in figure 52.

7. Press  to delete the value shown.

- » The display will then show the message **clear?** (figure 53).

8. Confirm by pressing .

- » The value has been deleted.



6. Calibration curves

Product name	Calibration curve	Compressed density	Measuring range
Straw round bales	Straw round bales	> 130 kg/m ³	8.5 % - 30 %
Straw bales	Straw rectangle bales	100 - 130 kg/m ³	8.5 % - 30 %
Straw loose	loose straw		8.5 % - 30 %
Hay round bales	Hay round bales	> 130 kg/m ³	8.5 % - 25 %
Hay bales	Hay rectangle bales	100 - 130 kg/m ³	8.5 % - 25 %
Hay loose	loose hay		8.5 % - 25 %
Cellulose	Insulating material - special product	38 - 65 kg/m ³	10 % - 35 %
Empty 1	free curve for special products		
Empty 2	free curve for special products		
Digit			0 - 100
Reference	! Only for testing the moisture meter !		

- » A divergent compressed density may lead to deviations in the measuring result.

6.1 Digit calibration curve

The Digit calibration curve has a unitless measuring range from 0 to 100, which corresponds to the entire measuring range of the device. Special materials can be measured with this calibration curve.

The higher the displayed value, the wetter the material. With the aid of a comparative measurement taken with a reference procedure, a table of comparative values can be created.

very dry: 0%

very wet: 100%

6.2 How moisture is defined

The device measures and shows the material moisture content. The moisture content readings are calculated in relation to the material's overall mass:

$$\%WG = \frac{M_n - M_t}{M_n} \times 100$$

M_n : Mass of the sample with average moisture content

M_t : Mass of the sample with zero moisture content

%WG: Moisture content (in accordance with EN ISO 18134-2)

6.3 Selecting the calibration curve

If you are not sure which calibration curve is the best suited for your material, it is recommended to carry out a reference measurement by kiln-drying (EN ISO 18134-2).

Schaller Messtechnik GmbH will be happy to advise you on the selection of the right calibration curve for special hay and straw types.

The insertion direction for both round and rectangle bales is from the face side of the bale as shown on the following figures. Measurements taken from any other direction may lead to incorrect readings.

Straw round bales



Straw rectangle bales



Hay round bales



Hay rectangle bales



Hay loose

58



Incorrect measurement

59



6.4 Notes for comparative measurement with oven-drying method

The device uses a much higher sample quantity than the drying oven (12-fold to 20-fold quantity of kiln-drying method). Furthermore, to determine a more accurate average moisture value in case of inhomogeneous material, there can be effected several measurements within a short time.

Considering a sampling error due to the considerably smaller sample quantity as well as the content of volatile matters (resin etc.) that are not water, the kiln-drying method will practically reach an accuracy of approx. $\pm 3\%$. Therefore, if the measuring values of these two very different methods of determining the water content are compared, differences of $\pm 3\%$ can be considered to be normal.

In the standard EN ISO 18134-2 is declared that the drying oven method provides no absolute values, but only comparable values.


7. Using the LogMemorizer program

To do so: The device is provided with USB interface, and the USB stick with LogMemorizer software and USB cable are available. Otherwise, you can also install the software at humimeter.com/software or by scanning the QR code.



7.1 Installing / opening the program

1. Insert the USB stick with the LogMemorizer program into the USB port on your computer or
 - » download the LogMemorizer software at humimeter.com/software or use the QR code.
2. Open the **setup** application.
3. Follow the installation instructions.
4. Open LogMemorizer.
 - » The screen will now display the LogMemorizer's interface (figure 60).

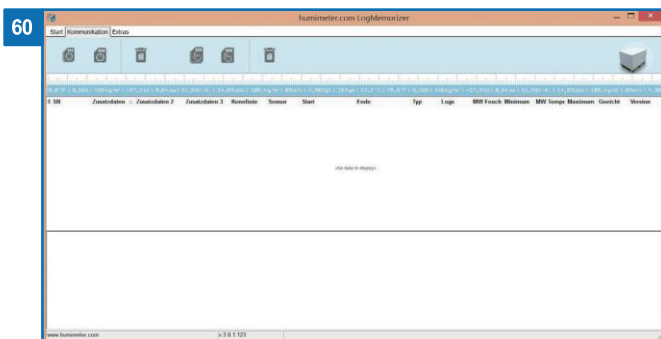

- » Before using LogMemorizer, please refer to the the separate LogMemorizer operating manual for the correct configuration of the USB COM Port.

For more information on LogMemorizer, please refer to the separate LogMemorizer operating manual supplied with the device.








7.2 Exporting measured values to a computer



To do so: The LogMemorizer program is installed. You must have taken and saved one or several moisture readings.

Options: You can export moisture readings from the humimeter FL2 or initiate the export at your computer.

Exporting moisture readings from the humimeter FL2

Connect the humimeter FL2 to your computer using the supplied USB cable:

1. Insert the USB Mini B connector into the humimeter FL2 (figure 61).
 2. Insert the USB connector into the computer.
 3. Open LogMemorizer on your computer.
 4. Switch on the humimeter FL2.
 5. Press  twice or hold for 2 seconds.
 6. Select **Send Logs** (figure 62). To do so, press  or  and confirm by pressing .
 7. Select **Manual Logs** (figure 63). To do so, press  or  and confirm by pressing .
- » The display will then show the message **Send** (figure 64).
 - » All measuring values saved on the humimeter FL2 will now be sent to your computer.




Initiating the data export at your computer

Connect the humimeter FL2 to your computer using the supplied USB cable:


1. Insert the USB Mini B connector into the humimeter FL2 (figure 65).
2. Insert the USB connector into the computer.
3. Open LogMemorizer on your computer.



4. Switch on the humimeter FL2.
5. Open the **Communication** tab in LogMemorizer (figure 66).

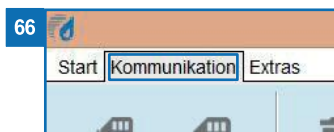



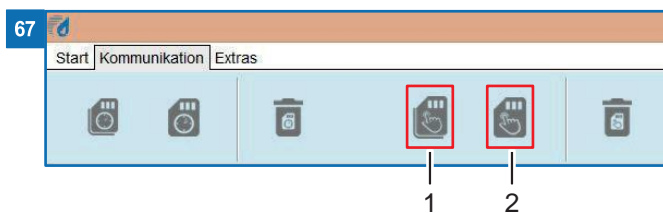

6. Select and click on one of the two buttons shown in figure 67.
 - » **Import all manual logs** (for importing all manually saved readings) **or**
 - » **Import most recent manual log** (for importing the most recent manually saved logs).



No	Name
1	Import all manual logs
2	Import most recent manual log



- » The measuring values saved on the humimeter FL2 will now be sent to your computer.

8. Checking on the device's status

1. Press  twice or hold for 2 seconds.
2. Select **Status**. To do so, press  or  and confirm by pressing .
 - » The display will then show the status indicator **humimeter**.
 - » The display will show the following information:



No	Name
1	Serial number
2	Software version
3	Battery status
4	Memory status








3. Confirm by pressing .
4. Press  to leave the main menu.



9. Configuring the device


9.1 Turning on Bluetooth





The information on Bluetooth is provided in a separate operating manual.



9.2 Adjust the date/time

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Date/Time**. To do so, press  or  and confirm by pressing .
 - » The display will now appear as shown in figure 68.
 - » The format for the date is **DD-MM-YY** (Day-Month-Year).
 - » The format for the time is **hh:mm:ss** (Hour:Minutes:Seconds).
4. **Inputting numbers:**













Press and hold  to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number (figure 69).
5. **Moving forward:**

To move forward between **DD-MM-YY** and **hh:mm:ss**, press .
6. **Moving back:**

Press  to switch to another input level. To move backward between **DD-MM-YY** and **hh:mm:ss**, press .
7. Confirm the date/time by pressing **OK**.
 - » The settings have been saved.
8. Press  to leave the **Options** menu.
9. Press  to leave the main menu.
















9.3 Selecting a language

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Language**. To do so, press  or  and confirm by pressing .
4. Navigate to the required language. To do so, press  or  and confirm by pressing .
- » The settings have been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.



9.4 Activating options

To do so: Some of the options must be deactivated.

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Unlock**. To do so, press  or  and confirm by pressing .
- » The display will now appear as shown in figure 70.
- » On delivery, the four-digit password is the device's serial number.
4. **Inputting numbers:**
Press and hold  to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number (figure 71).
5. **Moving back:**
Press  to switch to another input level.
To move back, press .
6. Confirm the four-digit password by pressing **OK**.



-
- » The settings have been saved.
 - » The **°C/°F**, **BL On Time**, **Auto Off Time**, **Materialcalib.**, **Password**, **Reset** options are now activated.













7. Press  to leave the **Options** menu.
8. Press  to leave the main menu.

9.5 Deactivating options

Once the device has been switched restarted, the **°C/°F**, **BL On Time**, **Auto Off Time**, **Materialcalib.**, **Password**, **Reset** options will be deactivated again.

9.6 Selecting °C/°F










To do so: All of the options must be activated (see "9.4 Activating options").

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **°C/°F**. To do so, press  or  and confirm by pressing .
4. Navigate to the required temperature scale, i.e. Celsius (**°C**) or Fahrenheit (**°F**). To do so, press  or  and confirm by pressing .
- » The settings have been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

9.7 Changing the Userlevel








9.7.1 Changing from advanced to simplified user

To do so: All of the options must be activated (see "9.4 Activating options").

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Userlevel**. To do so, press  or  and confirm by pressing 
 - » The simplified user is now activated.
4. Press  to leave the **Options** menu.
5. Press  to leave the main menu.

9.7.2 Changing from simplified to advanced user













To do so: The device has to be turned off.

1. Switch the device on (see "4.1 Switching the device on").
2. Press and hold  and  at the same time, directly after switching the device on.
 - » The device will automatically boot into the main menu.
3. Activate all of the options (see "9.4 Activating options").
4. Select **Userlevel**. To do so, press  or  and confirm by pressing 
 - » The advanced user is now activated.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

9.8 Reducing the device's power consumption













9.8.1 Configuring the display illumination time

To do so: All of the options must be activated (see "9.4 Activating options").

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **BL On Time**. To do so, press  or  and confirm by pressing .
4. Select the required display illumination period (30 seconds/2 minutes/5 minutes/10 minutes). To do so, press  or  and confirm by pressing .
- » The settings have been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

9.8.2 Configuring automatic switch-off

To do so: All of the options must be activated (see "9.4 Activating options").









1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Auto Off Time**. To do so, press  or  and confirm by pressing .
4. Select the period of time you want the device to stay switched on (3 minutes/5 minutes/10 minutes). To do so, press  or  and confirm by pressing .
- » The settings have been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

9.9 Configuring the material calibration function


The type calibration function is described in a separate operating manual.

9.10 Changing the password



To do so: All of the options must be activated (see "9.4 Activating options").

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Password**. To do so, press  or  and confirm by pressing .
 - » The display will show the current password.
 - » Overwrite the current password. To do so, press and hold **0..9** to quickly scroll to the required number and either press it for 3 seconds or press  to confirm the selected number.

Moving back:









Press  to switch to another input level.

To move back, press .

4. Confirm the new four-digit password by pressing **OK**.
 - » The settings have been saved.
5. Press  to leave the **Options** menu.
6. Press  to leave the main menu.

9.11 Resetting the device to its factory settings

To do so: All of the options must be activated (see "9.4 Activating options").

1. Press  twice or hold for two seconds.
2. Select **Options**. To do so, press  or  and confirm by pressing .
3. Select **Reset**. To do so, press  or  and confirm by pressing .
- » The display will then show the message **Reset?** (figure 72).
4. Confirm by pressing .
- » The device will now be reset to its factory settings. All of your personal settings will be lost.
- » The display will show the status indicator **humimeter** (figure 73).
- » Resetting the device will not affect the saved measuring values.



10. Cleaning and maintenance

Regularly cleaning and maintaining the device will ensure that it will have a long service life and stay in good condition.


10.1 Changing batteries

The device constantly monitors the charge level of the batteries. The current battery status is shown on the status screen.

If the battery's charge is very low, the battery symbol will be shown with an exclamation mark. In that case, the batteries must be changed immediately (figure 75).

For changing the batteries, see section "3.3 Inserting batteries".

As the device's user, you are responsible by law for properly disposing of all used batteries, which must not be disposed of as domestic waste (Battery Directive).



10.2 Care instructions

- Do not leave the device out in the rain. The device is not waterproof.
- Do not expose the device to extreme temperatures.
- Protect the device from strong mechanical shocks and loads.

10.3 Cleaning the device

Plastic housing

- Clean the plastic housing with a dry cloth.

Measuring head

- The measuring head can be cleaned with a cloth and cleaning alcohol.



ATTENTION

Do not clean with fluids

Water or cleaning fluid getting inside the device can destroy the device.

- ▶ Only clean with dry materials.

11. Faults

If the measures listed below fail to remedy any faults or if the device has faults not listed here, please contact Schaller Messtechnik GmbH.

Fault	Cause	Remedy
Measuring error	The temperature of the material being measured is too low or high	The temperature of the material being measured has to be between 0 °C and +40 °C.
	Temperature discrepancy between device and material being measured	Let the temperature adjust to the material being measured (permitted difference of max. 3 °C).
	Wrong calibration curve	Check whether you have selected the right calibration curve (product) before taking a reading (see "6. Calibration curves").
	Mouldy or rain wet material Accuracy decreases significantly	Only measure dry, not mouldy material.
	Frozen material or material mixed with snow Accuracy decreases significantly	The measured material must not be frozen or mixed with snow.
	Insertion direction	The insertion direction has a great effect on the accuracy of the measurement (see "6.3 Selecting the calibration curve").
	Wrong compressed density	The compressed density has to correspond to the selected calibration curve(see "6. Calibration curves").

Fault	Cause	Remedy
	Water film on the measuring head	After measuring wet material, on the measuring head may arise a water film. Clean the measuring head (see " 10.3 Cleaning the device ").
	Heating of the measuring head because of friction in bales with high compressed density	Let the device cool down.
Data transfer to Log Memorizer failed	Interface has not been configured.	The interface only has to be configured once. To do so, press the F1 key on your computer and read the Help file of the Log Memorizer program.

12. Storage and disposal

12.1 Storing the device

The device must be stored as follows:

- Do not store outdoors.
- Store in a dry and dust-free place.
- Protect the device from sunlight.
- Avoid mechanical shocks/loads.
- Remove the batteries if the device isn't used for a period of 4 weeks or longer.
- Store the device in its original packaging if it isn't used for a longer period of time.
- Storage temperature: -20 °C to +60 °C

12.2 Disposing of the device



Devices marked with this symbol are subject to Directive 2012/19/EU of the European Parliament and of the Council of 4 July 2012 on waste electrical and electronic equipment (WEEE).

If the device is being operated outside the European Union, the national regulations on the disposal of such devices that apply in the country of use must be observed.

Electronic devices must not be disposed of as domestic waste.

The device must be disposed of appropriately using appropriate collection systems.

13. Device information

13.1 CE declaration of conformity



Name/ Adresse des Herstellers: <i>Name/ address of manufacturer:</i>	Schaller Messtechnik GmbH Max-Schaller-Straße 99 A – 8181 St. Ruprecht
Produktbezeichnung: <i>Product designation:</i>	humimeter
Typenbezeichnung: <i>Type designation:</i>	BL2 ; BLL ; BLH ; BLW ; FL1 ; FL2 ; FLH ; FLM ; FLS ; RM1 ; SLW ; WLW
Produktbeschreibung: <i>Product description</i>	Messgerät zur Bestimmung des Wassergehalts in Biomasse und diversen Schüttgütern <i>Measuring device for determining the water content in bio- mass and various bulk materials</i>

Das bezeichnete Produkt erfüllt die Bestimmungen der Richtlinien:
The designated product is in conformity with the European directives:

EMV - Richtlinie 2014/30/EC	EMC Directive 2014/30/EU
RoHS - Richtlinie 2011/65/EG	RoHS-Directive 2011/65/EU

Die Übereinstimmung des bezeichneten Produktes mit den Bestimmungen der Richtlinien wird durch die vollständige Einhaltung folgender Normen nachgewiesen:

Full compliance with the standards listed below proves the conformity of the designated product with the provisions of the above-mentioned EC Directives:

EN 61326–1:2013	Elektrische Mess-, Steuer-, Regel- und Laborgeräte - EMV-Anforderungen <i>Electrical equipment for measurement, control, and laboratory use – EMC requirements</i>
EN IEC 63000:2019-05 <i>ersetzt / replaced</i> EN 50581:2012	Technische Dokumentation zur Beurteilung von Elektro- und Elektronikgeräten hinsichtlich der Beschränkung gefährliche Stoffe. <i>Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances.</i>

Für das angeführte Produkt ist eine vollständige Dokumentation mit Betriebsanleitung in Originalfassung vorhanden.

For the mentioned product a complete documentation with manual of instruction in original version is available.

Bei Änderungen, die nicht vom Hersteller spezifiziert sind, verliert diese Konformitätserklärung die Gültigkeit.

In case of any changes not agreed upon with the manufacturer, this declaration of conformity loses its validity.

St. Ruprecht a.d. Raab, 31.07.2022

 **Schaller**
Messtechnik / filmeter.com
Schaller Messtechnik GmbH
Mes - Schaller - St. Ruprecht a.d. Raab
AT - 8190 St. Ruprecht a.d. Raab
www.filmeter.com | info@filmeter.com
.....
Bernhard Maunz
Rechtsverbindliche Unterschrift des Ausstellers
Legal binding signature of the issuer



DECLARATION OF CONFORMITY

Name/ address of manufacturer: **Schaller Messtechnik GmbH**
Max-Schaller-Straße 99
A – 8181 St. Ruprecht

Product designation: **humimeter**

Type designation: **BL2 ; BLL ; BLH ; BLW ; FL1 ; FL2 ; FLH ; FLM ; FLS ; RM1 ;
SLW ; WLW**

Product description: **Measuring device for determining the water content in bio
mass and various bulk materials**

The designated product is in conformity with the following directives:

- **Electromagnetic Compatibility Regulations 2016 Great Britain**
- **RoHS-Directive 2011/65/EU Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment**


Full compliance with the standards listed below proves the conformity of the designated product with the provisions of the above-mentioned Directives:

EN 61326–1:2013	Electrical equipment for measurement, control, and laboratory use – EMC requirements
EN IEC 63000:2019-05 replaced EN 50581:2012	Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances.

For the mentioned product, a complete documentation with manual of instruction in original version is available.

In case of any changes not agreed upon with the manufacturer, this declaration of conformity loses its validity.


St. Ruprecht a.d. Raab, 31.07.2022




Schaller
Messtechnik / www.humimeter.com
Schaller Messtechnik GmbH
Maunz - Schaller Straße 199
AT-8187 St. Ruprecht a.d. Raab
www.humimeter.com | info@humimeter.com
.....
Bernhard Maunz
Legal binding signature of the issuer

13.2 Technical data

Display resolution	0.1 % moisture content, 0.5 °C/°F temperature
Measuring range	8 % to 30 % water content
Operating temperature	0 °C to +40 °C
Temperature measuring range	-20 °C to +120 °C (only measuring head)
Storage temperature	-20 °C to +60 °C
Temperature compensation	Automatic
Data memory	Up to 10,000 measuring values
Power supply	4 pcs. of 1.5 Volt AA Alkaline batteries
Current consumption	60 mA (incl. display illumination)
Menu languages	English, German, French, Italian, Spanish, Portuguese, Czech, Polish, Russian, International
Display	128 x 64 illuminated matrix display
Device dimensions	740 x 65 x 40 mm
Device weight	450 g (with batteries)
Device IP rating	IP 40





GRUBATEC



MESS- UND REGELTECHNIK

Gewerbehaus Ergolz, Wölferstrasse 5
4414 Füllinsdorf

Telefon: +41 (0)55 617 00 80

Telefax: +41 (0)55 617 00 81

www.grubatec.ch
sales@grubatec.ch